

1/3

ION SOURCE	MASS SPECTROMETER
<u>20</u>	<u>30</u>

FIG. 1

2/3

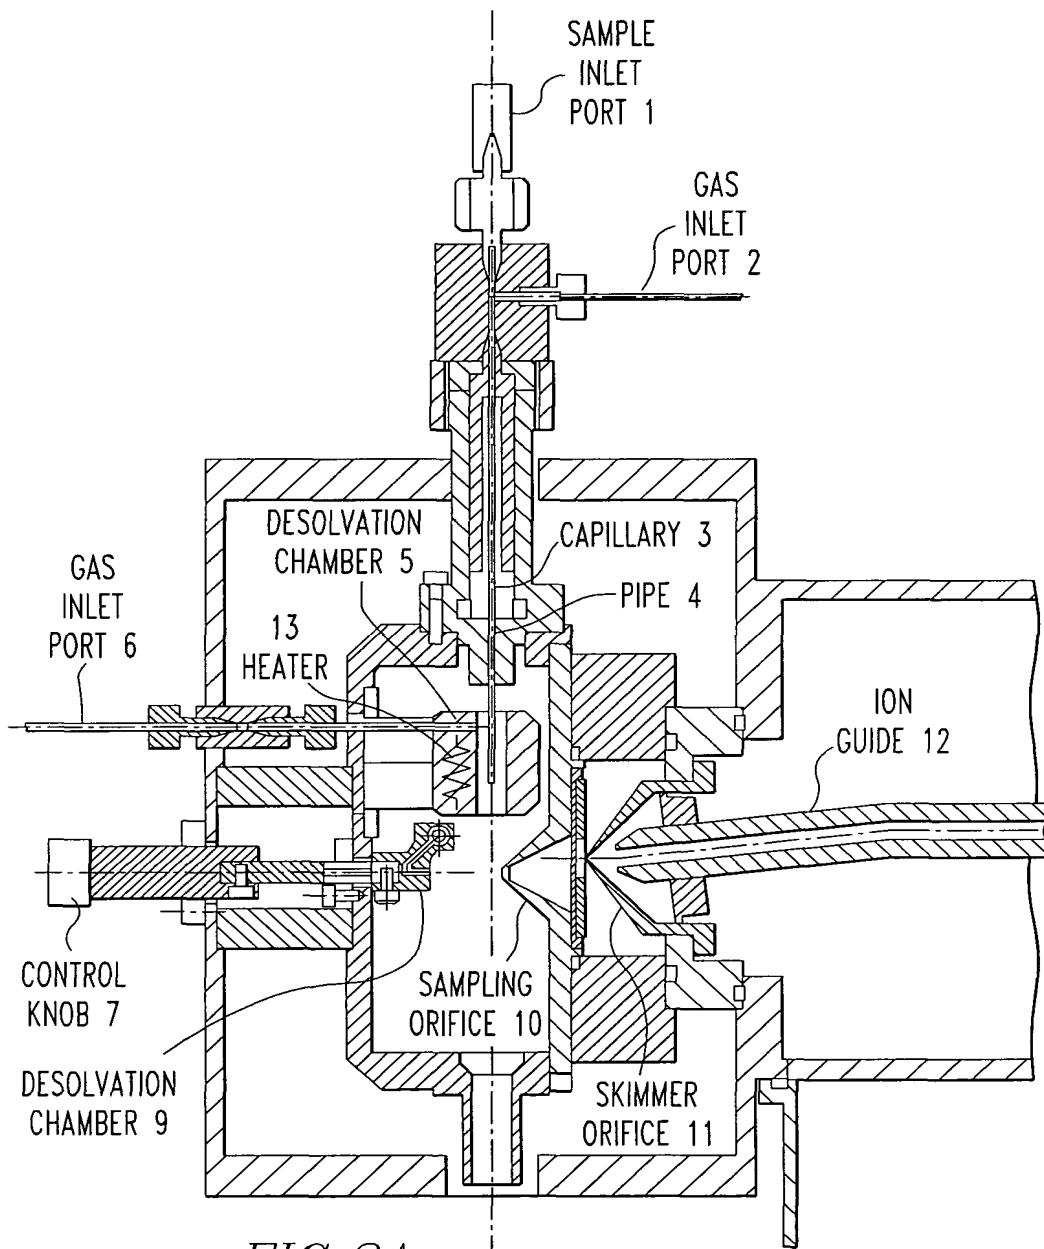


FIG. 2A

3/3

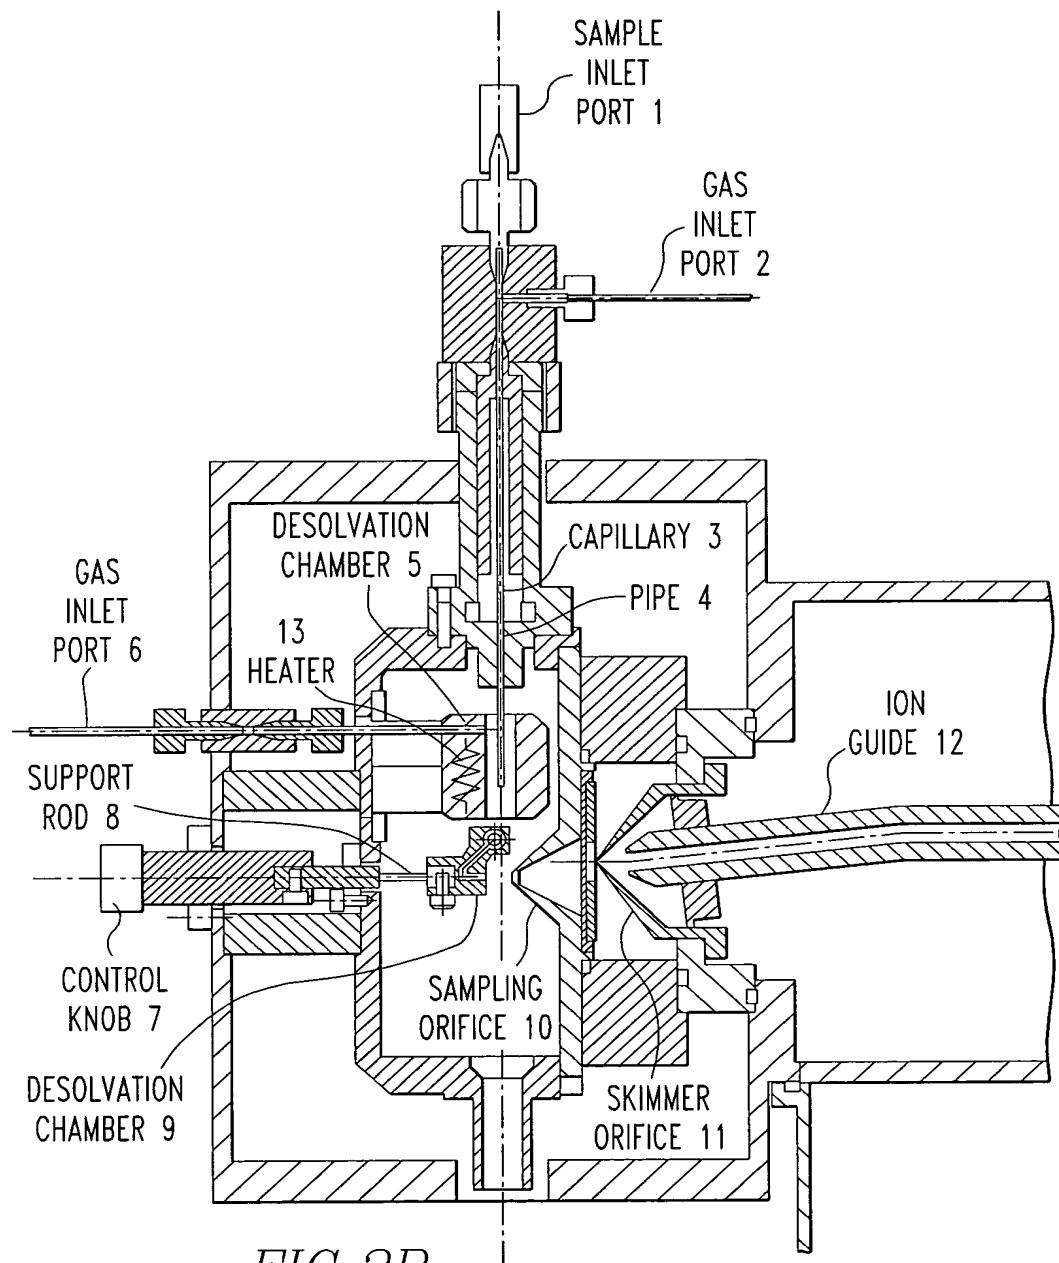


FIG. 2B